




Disinfection, Decontamination and Deodorization Solution

biotekozone




Biotek Ozone Disinfection System

| | | |
|-----------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------|
| <p>Countertop/Wall Mount Model</p> <p>C-7120 / C-7120U</p>  | <p>Central Water Treatment Model</p> <p>CDS</p>  | <p>Mobile Model</p> <p>MDS</p>  |
|-----------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------|

 **Accessory - Spray Bottle**
 The aluminum ally spray bottle is designed for surface disinfection, e.g. kitchen worktop, food counter etc. Its inner layer was coated with epoxy resin, which is antioxidant material, and thus it can store 275 ml of high concentrated ozone water (2-4ppm) and can keep for approx. 20-40 mins.

Application of Biotek Ozone Disinfection System

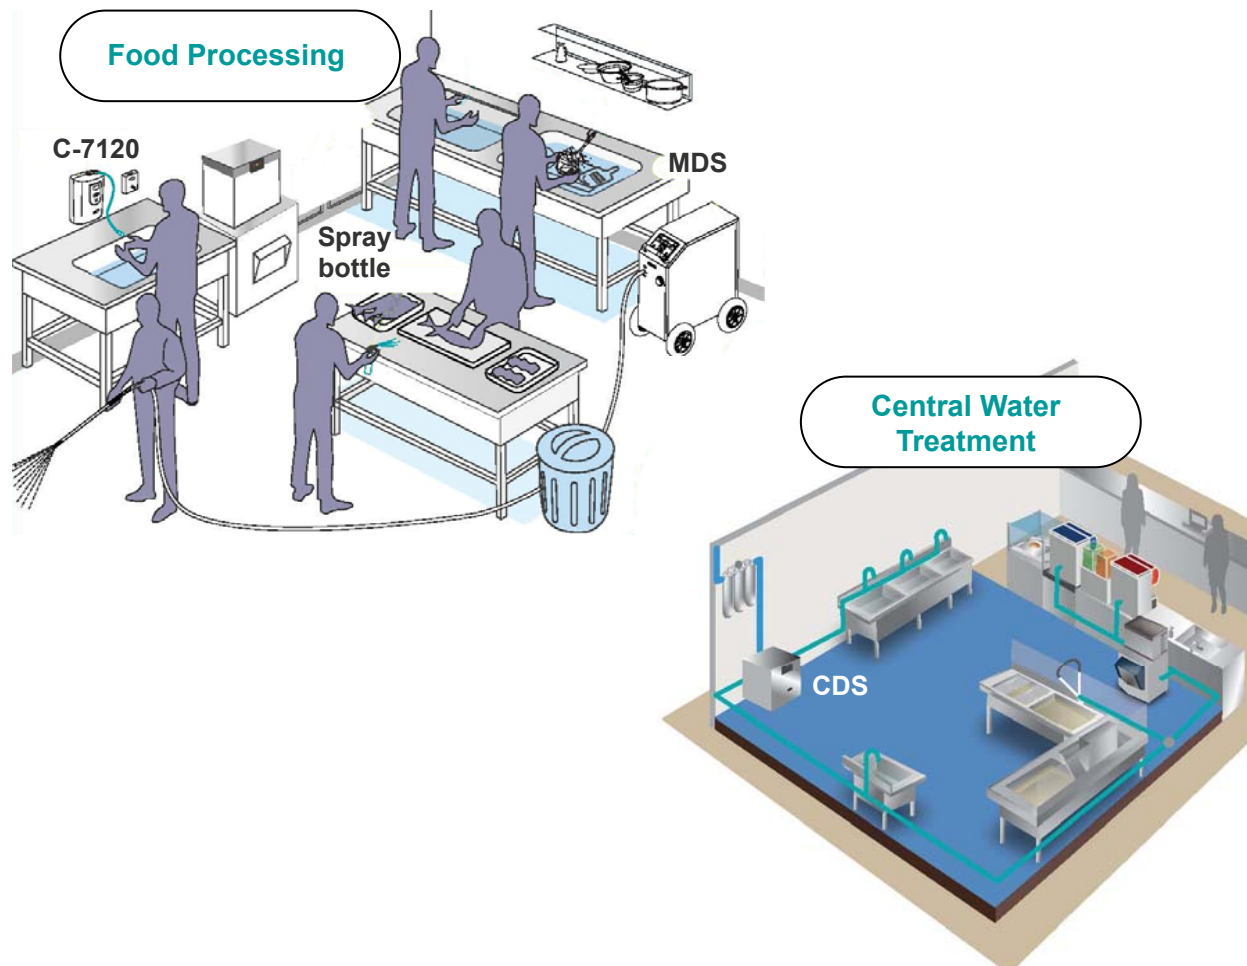



Biotek Ozone Disinfection System Specifications

| Model | C-7120 | C-7120U | CDS | MDS |
|------------------------------|--------------------------------------------------------------|------------|----------------------------|----------------------------|
| Type | Countertop | Under-sink | Floor | Mobile |
| Color | Dark grey | | Stainless steel | Stainless steel |
| Flow rate | 180±10% L/hr | | 100-3000 L/hr | 400-3000 L/hr |
| O ₃ concentration | 4 ppm (0-20 sec.) 2 ppm (0-20 min.) 1 ppm (continuous) | | 0.2-6.0 ppm | 0.5-6.0 ppm |
| Input Press | 1.5-7.0 kg/cm ² | | 2.0-4.0 kg/cm ² | 2.0-7.0 kg/cm ² |
| Output Press | 0.1-0.3 kg/cm ² | | ≤3.0 kg/cm ² | 1.5-3.0 kg/cm ² |
| Ozone generator life | 3,000 hrs | | 6,000 hrs | 6,000 hrs |
| Elect. loading | 220V /50h / 1ph; 800W | | 220V /50h / 1ph; 800W | 220V /50h / 1ph; 950W |
| Dimension | 330 x 190 x 410 mm (H) | | 400 x 700 x 709 mm (H) | 420 x 1000 x 900 mm (H) |

ppm (parts per million) is used to measure concentration.
 1 ppm = 1 mg/liter, i.e. 1 milligram of dissolved ozone molecules in 1 liter of ozone water solution.

Biotek's Ozone Generation Technology


In the past 15 years, Biotek has developed its **Electrolytic Ozone Generator** and its integrated ozone system has obtained more than 40 patents. Its technology is to **create ozone from water into water** for application, i.e. using normal tap water, going through the Biotek's electrolytic ozone generator, **generating 20% to 30% ozone to be dissolved in water** via its injection system, thus providing instant high concentration ozonated water.

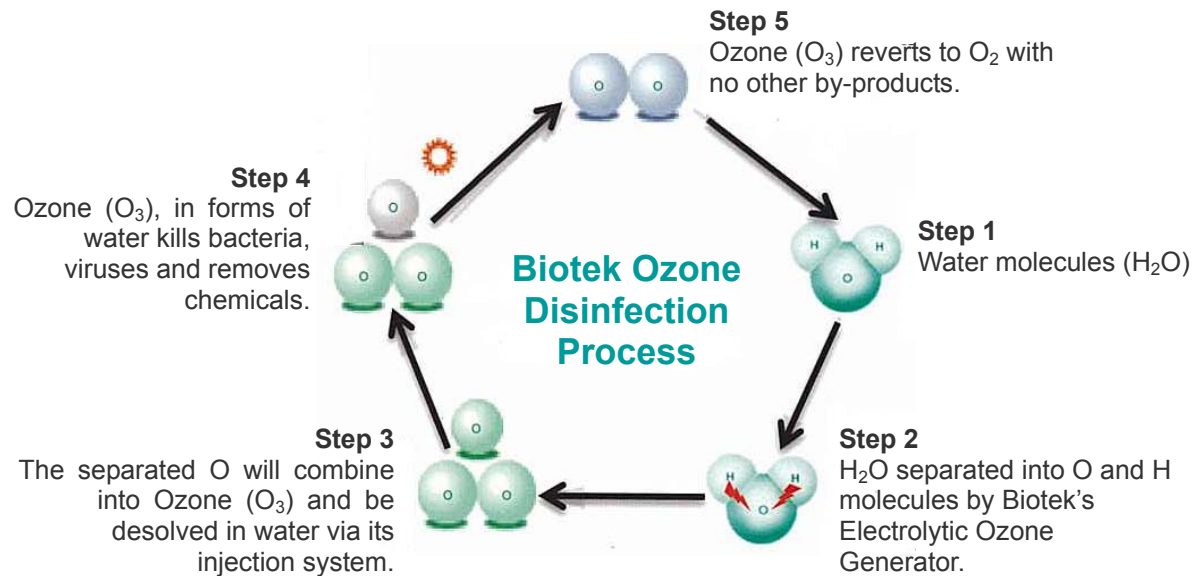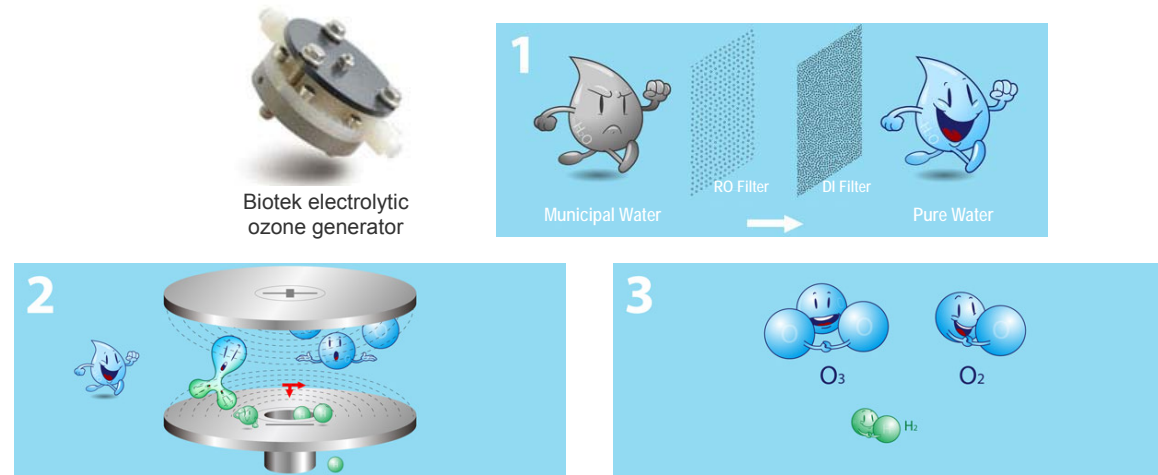

Test Reports on Effectiveness of Biotek Ozone Water

| SGS Test Report of Biotek Ozone Water Disinfection (2.0 ppm O ₃) | | | | | |
|------------------------------------------------------------------------------|---------------------------------|---------------------|--------------|--------------|-----------|
| Test Item | | 0 sec. | 5 sec. | 15 sec. | Reduction |
| Antimicrobial Effectiveness Testing | Staphylococcus aureus (CFU/ml) | 5.4x10 ⁵ | Not detected | Not detected | >99.999% |
| | Escherichia coli (CFU/ml) | 2.5x10 ⁵ | 6.1x10 | <10 | 99.99% |
| | Salmonella (CFU/ml) | 1.7x10 ⁵ | 1.9x10 | Not detected | 99.9% |
| | Pseudomonas aeruginosa (CFU/ml) | 4.5x10 ⁵ | Not detected | Not detected | >99.999% |
| | Candida albicans (CFU/ml) | 1.3x10 ⁵ | Not detected | Not detected | >99.999% |
| | MRSA (CFU/ml) | 1.3x10 ⁵ | Not detected | Not detected | >99.999% |
| Decomposition of Residual Pesticide | Mevinphos | 0.642 | 0.0000 | | 100% |
| | Permethrin | 0.559 | 0.0337 | | 94% |

Biotek Ozone Water vs. Chlorine – Difference Testing on Disinfection Effectiveness (Test conducted by SGS)

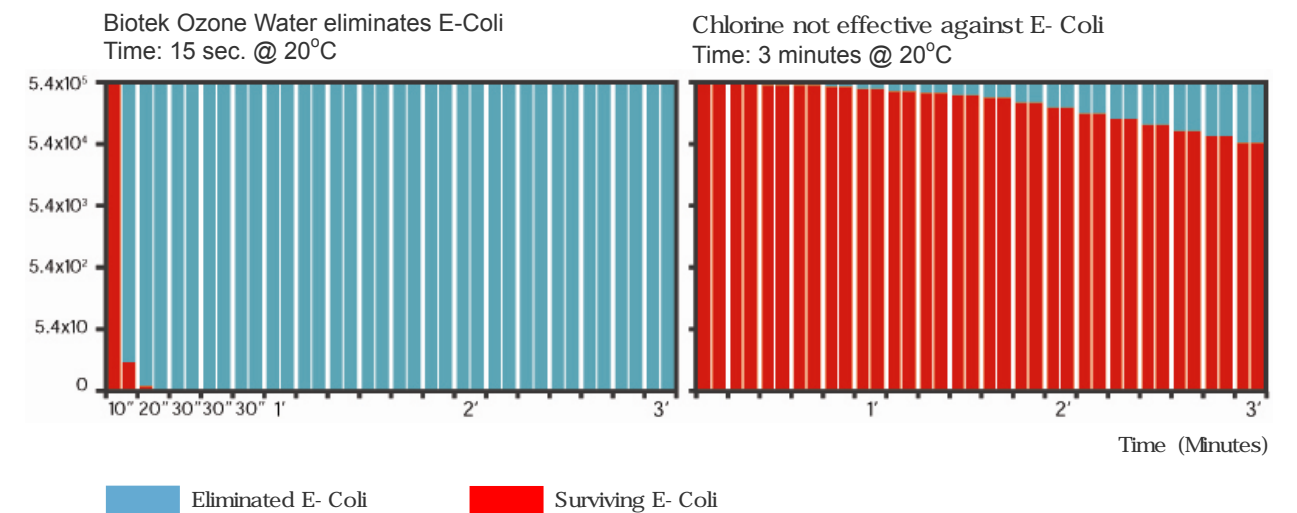

Product – Technology

List of Micro-organisms Disinfected by Biotek Ozone Water

BACTERIA

| | | |
|--------------------------------|--------------------------------|------------------------------------|
| Achromobacter butyric NCI-9404 | Escherichia coli | Serratia marcescens |
| Aeromonas harveyi NC-2 | Flavobacterium SP A-3 | Shigella dysenteriae |
| Aeromonas salmonicida NC-1102 | Leptospira canicola | Shigella flexneria |
| Bacillus anthracis | Listeria | Shigella paradysenteriae |
| Bacillus cereus | Micrococcus candidus | Spirillum rubrum |
| B. coagulans | Micrococcus caseolyticus KM-15 | Staphylococcus albus |
| Bacillus globigii | Micrococcus sphaeroides | Staphylococcus aureus |
| Bacillus licheniformis | Mycobacterium leprae | Streptococcus 'C' |
| Bacillus megatherium sp. | Mycobacterium tuberculosis | Streptococcus faecalis |
| Bacillus paratyphosus | Neisseria catarrhalis | Streptococcus hemolyticus |
| B. prodigiosus | Phytomonas tumefaciens | Streptococcus lactis |
| Bacillus subtilis | Proteus vulgaris | Streptococcus salivarius |
| B. stearothermophilus | Pseudomonas aeruginosa | Vibrio alginolyticus & anguillarum |
| Clostridium tetoni | Salmonella choleraesuis | Vibrio cloarae |
| Cryptosporidium | Salmonella enteritidis | Vibrio comma |
| Coliphage | Salmonella typhimurium | Virrio ichthyodermis NC-407 |
| Corynebacterium diphthriae | Salmonella typhosa | V. parahaemolyticus |
| Eberthella typhosa | Salmonella paratyphi | |
| Endamoeba histolica | Saricna lutea | |

VIRUS

| | | |
|-------------------------|----------------------|-------------------------------------|
| Adenovirus (type 7a) | Encephalomyocarditis | Legionella pneumophila |
| Bacteriophage (E. coli) | Hepatitis A | Polio virus (Polimyelitus) 1, 2 & 3 |
| Coxsackie A9, B3, & B5 | HIV | Rotavirus |
| Cryptosporidium | GD V11 Virus | Tobacco mosaic |
| Coronavirus (SARS) | Onfectious hepatitis | |
| Echoviurs 1, 5, 12 & 29 | Influenza | |

FUNGUS & MOLD SPORES

| | | |
|--------------------------------------|----------------------------------|--------------------------------|
| Aspergillus candidus | Fusarium oxysporum | Penicillium digitatum (olive) |
| Aspergillus flavus (yellowish-green) | Grotrichum | Penicillium glaucum |
| Aspergillus glaucus (bluish-green) | Mucor recomosus A&B (white-gray) | Pennicillium expansum (olive) |
| Aspergillus niger (black) | Mucor piriformis | Penicillium egyptiacum |
| Aspergillus terreus, saitoi & oryzac | Oospora lactis (white) | Penicillium roqueforti (green) |
| Botrytis allii | Penicillium cyclopium | Rhizopus nigricans (black) |
| Colletotrichum lagenarium | P. chrysogenum & citrinum | Rhizopus stolonifer |

Product – Technology

Biotek Ozone Water vs Common Disinfection Methods

| Application Comparisons | | | | | |
|-------------------------|--------------------|-------------|-----------------|------------------|--------------|
| | Biotek Ozone Water | Alcohol Gel | Liquid Chlorine | Chlorine Dioxide | Heat & Steam |
| Hand sanitation | √ | √ | √ | √ | × |
| Produce wash | √ | × | √ | √ | × |
| Utensil disinfection | √ | × | √ | √ | √ |
| Surface disinfection | √ | × | √ | √ | × |
| Deodorizing | √ | × | × | × | × |
| Pre-storage rinse | √ | × | × | × | × |

| Operation Comparisons | | | | | |
|------------------------------|--------------------|--------------|-----------------|------------------|--------------|
| | Biotek Ozone Water | Alcohol Gel | Liquid Chlorine | Chlorine Dioxide | Heat & Steam |
| Efficacy | highest | medium / low | medium | medium / high | medium / low |
| No chemical residues | √ | × | × | × | √ |
| Initial cost | high | low | low | low | high |
| Running cost | low | medium | medium | medium | medium |
| Free from chemical storage | √ | × | × | × | √ |
| Reliable efficacy | √ | × | × | × | × |
| Safe operation | √ | × | × | × | × |
| Simple use | √ | √ | × | × | × |
| Fast effectiveness <10 mins. | √ | × | × | × | × |
| Energy/water expenditure | low | low | high water | high water | high |

| Effectiveness and Convenience Comparisons | | | | | |
|--------------------------------------------------------------|--------------------|-------------|-----------------|------------------|--------------|
| | Biotek Ozone Water | Alcohol Gel | Liquid Chlorine | Chlorine Dioxide | Heat & Steam |
| Effective on bacteria | √ | √ * | √ * | √ * | √ |
| Effective on viruses | √ | × | × | × | × |
| Effective on pesticides | √ | × | × | × | × |
| Residual disinfection | √ ** | √ | √ | √ | × |
| Compatible with all materials (including raw food materials) | √ | × | × | × | √ |
| Extend shelf time | √ | × | × | × | √ |
| Environmentally friendly | √ | × | × | × | √ |

* Effective in lab controlled test but proven to be inconstant in practical applicaiton

** Ozone has a residence time of 20 mins. Biotek ozone water will provide disinfection more than 10 mins. after output.

Product – Technology

Certifications of Biotek

Biotek has engaged in research and development of electrolytic ozone generator technology for more than two decades and obtained more than 40 international patents, including 12 PCT patents. Its high purification performance has been approved by many international standard inspections and testings.



NSF (National Sanitation Foundation)

NSF is committed to protect the public safety and environment. It is an independent, non-profit organization that develops standards and certifies products for the world's food, water and consumer goods. The standard of NSF is being recognized worldwide.

Biotek is the only ozone generator that has been approved in the official list of NSF169 – Special Purpose Food Equipment and Devices.



HACCP Australia – Hazard Analysis and Critical Control Points

HACCP Australia is a leading food science organization specializing in the HACCP Food Safety Methodology and its applications within the food and related food industries.

Biotek has been endorsed as “Food-Safe” sanitation for food processing facilities.



SGS

SGS is the world's leading inspection, verification, testing and certification company and recognized as the global benchmark for quality and integrity.

Biotek has passed various tests conducted by SGS on its effectiveness of disinfection on different micro-organisms.



OSHA – Occupational Safety and Health Administration

OSAH aims to assure safe and health working conditions by setting and enforcing standards and also providing training, outreach and education.

Biote meets the U.S. OSHA's critical requirement for off-gas levels to be below 0.008 ppm/8 hr.

Product – Technology



FDA – Food and Drug Administration

FDA is responsible for protecting and promoting public health through the regulation and supervision of foods and drugs produced in the U.S. or imported from other countries.

Ozone is approved to be safe for use as an antimicrobial agent on food, including meat and poultry in 2001 by FDA.



Ministry of Health of the P.R.C.

Biotek has been tested and proved that Biotek's ozonated water complied with the standard for the use in medical disinfection.



The Academy of Military Medical Sciences (AMMS) of the P.R.C.

Biotek has passed various tests conducted by AMMS on its ozone concentration, effectiveness of disinfection on different micro-organisms etc.



ISO – International Standard Organization

ISO develops and uniforms worldwide industrial and commercial standards.

Biotek complied and obtained ISO9001:2000 Quality Management System and ISO13485:2003 Management systems standard specifically developed for the manufacture of medical devices.



CE and UL

CE is the uniform standard and regulation developed by European countries for safe operation of electrical products produced in EU or imported from other countries.

UL is an independent product safety testing and certification organization in the U.S.

Biotek complies with the essential requirements of both CE and UL in relevant health, safety, environmental protection legislations.

Applications

Application of Biotek Ozone Water



Hand Disinfection



Our hands come into contact with many different objects everyday and can be easily contaminated with bacteria and viruses and must be thoroughly cleaned before any food processing or eating.

Prewash hands with soap and rinse hands under ozone water for at least 20 seconds, **microorganisms on hands can be reduced by 71.4%**.

Floor / Utensil Surface Disinfection

Some chemicals are commonly used for floors and utensil surfaces, but not only these chemicals are ineffective to some bacteria and viruses, they are also harmful to be human body and the environment themselves.

Performing floors and utensil surface disinfection with ozone water will **eliminate up to 99.9999% of microorganisms and chemicals**, ensuring a clean and safe environment.

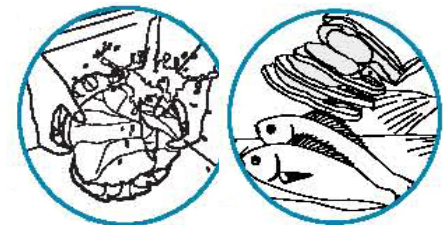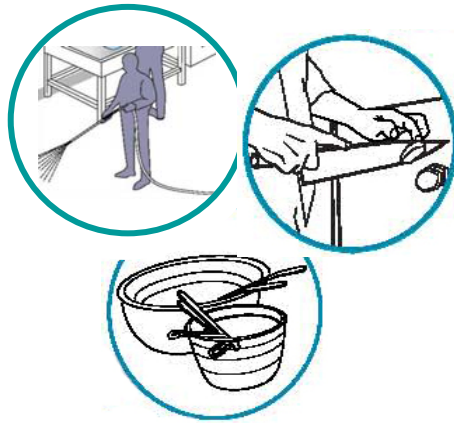

Food Disinfection and Preservation

Food safety has always been the most important criteria among all precaution procedures. It mainly involves cleaning processing and preserving.

Cleaning and processing food with ozone water will not only **minimize contamination and reduce microorganisms up to 99.9999%, it will also prolong the shelf life of food by as much as 200%**.

Ice Disinfection

Whether for drink or storage, ice is also an issue that cannot be overlooked.

Making ice with ozone water, the ices are **not only safely for eating, but also safe from contamination of foods** for storage so as to keep the freshness and shelf life of foods.



FAQ

Q: Is it safe to use Biotek?

A: It is absolutely safe. Biotek generates high concentrated ozonated water for eliminating pesticides, harmful chemicals, viruses and bacteria etc. It will naturally revert to oxygen, leaving no harmful by-products or residues. It is certified by OSHA in the USA, that the off-gas level of Biotek is below 0.008 ppm / 8 hrs.

Q: Biotek generates highly concentrated ozonated water for applications. However, will it be harmful to humans?

A: It has been tested and proved that there are no harmful effects on humans when applying 4 ppm ozonated water generated by Biotek onto human skin and fingers. Please refer to PSE Certification.

Q: What kind of bacteria and viruses as can be killed by Biotek's ozonated water?

A: Please view the list of micro-organisms that can be disinfected by Biotek's ozonated water.

Q: Can the ozonated water generated by Biotek be drunk?

A: Biotek is designed to be used for cleaning foods and tools, such as decomposing pesticides on fruits and veggies, sanitizing hands and kitchen wares before handling of foods, eliminating germs on seafood and meat for longer preservation. Therefore, it is not recommended for drinking.

Q: There is a traditional generation method named "Corona Discharge". How is it different from Biotek's?

A: The "Corona Discharge" method uses high voltage electrical discharges, giving energy to O₂ in the input air and to form ozone. However, the volume and concentration of ozone generated by this method will be affected by the quality, humidity and temperature of air. Also, only less than 0.5 ppm ozone can be dissolved in the water for applications and thus the effectiveness of disinfection is low. Moreover, there are the by-products of nitrogen oxides and dioxides (NO_x) which are harmful to human.

Biotek's electrolytic ozone generation technology uses normal tap water, goes through Biotek's electrolytic ozone generator, generates ozone to be dissolved in water via its injection system and provides instant high concentration ozonated water. After the oxidation process, ozone will revert to oxygen, leaving no harmful by-products or residues.



Distributor of Biotekozone in HK:
Total Nutrition Center Ltd.
Tel: (852) 2881-8270 Email: enquiry@tnc.com.hk
Website: www.tnc.com.hk